

POSTER PRESENTATION

Open Access

# High-dose dobutamine stress SSFP cine MRI at 3 Tesla with patient adaptive local RF shimming using dual-source RF transmission

Alexander Berger<sup>1\*</sup>, Bernhard Schnackenburg<sup>2</sup>, Christopher Schneeweis<sup>1</sup>, Sebastian Kelle<sup>1</sup>, Christoph Klein<sup>1</sup>, Marc Kouwenhoven<sup>3</sup>, Eckart Fleck<sup>1</sup>, Rolf Gebker<sup>1</sup>

From 15th Annual SCMR Scientific Sessions  
Orlando, FL, USA. 2-5 February 2012

## Background

Image quality of cine imaging using steady state free precession (SSFP) sequences at 3T is insufficient due to increased RF-inhomogeneity (B1 field) and the high sensitivity of SSFP sequences to off-resonance artefacts. Recently, the introduction of a dual source RF transmission system with patient-adaptive local RF-shimming has led to a significant improvement of image quality of SSFP imaging at 3T.

The objective of this study was to prospectively evaluate the feasibility, image quality and diagnostic accuracy of high-dose dobutamine stress magnetic resonance imaging (DSMR) at 3T comparing dual-source versus single-source transmit technology.

## Methods

DSMR was performed in 44 patients with each participant undergoing cine imaging at rest and during dobutamine infusion using both dual- and single-source transmit technology.

B1-maps and measurements of contrast to noise ratio (CNR) were evaluated to quantify the effect of RF calibration in both transmission modes.

Analysis of image quality (0=non diagnostic, 1=severe artifact, 2=slight artifact, 3=no artifact) and wall motion was performed at rest and at maximum stress comparing single- and dual-source technology.

CAD was defined on invasive coronary angiography as the presence of  $\geq 70\%$  stenosis.

## Results

The mean percentage of the intended flip angle within the heart increased from  $88\% \pm 9.1$  with single-source to  $103\% \pm 5.6$  with dual-source ( $p < 0.001$ ). Deviation of the flip angle from the base to the apex along the pseudo-long axis decreased from  $29.8\% \pm 12.9\%$  with single-source to  $12.8\% \pm 7.2\%$  with dual-source.

CNR increased for dual-source vs. single-source especially pronounced at the apex ( $63.4 \pm 24.2$  vs.  $36.5 \pm 16.5$ ,  $p < 0.001$ ) but also at the base ( $50.1 \pm 14.8$  vs.  $39.3 \pm 15.8$ ,  $p < 0.001$ ).

Image quality of dual-source was higher than single-source both at rest ( $2.8 \pm 0.5$  vs.  $2.6 \pm 0.7$ ,  $p < 0.001$ ) and stress ( $2.5 \pm 0.7$  vs.  $2.0 \pm 1.0$ ,  $p < 0.001$ ). The number of segments with either severe artifacts or non-diagnostic image quality at stress was 27% using single-source compared to only 8% using dual-source (figure 1).


No significant differences between dual-source DSMR and single-source DSMR were seen regarding sensitivity (92% vs. 83%,  $p = 0.38$ ) and specificity (88% vs. 50%,  $p = 0.25$ ) due to the relatively small patient cohort. Diagnostic accuracy of dual-source DSMR (90%) was significantly higher than single-source DSMR (77%) ( $p = 0.006$ ) (figure 2).

## Conclusions


We demonstrated that using a dual-source transmit technology in a standard DSMR protocol is feasible in a 3T environment. Furthermore, the dual-source transmit technology provides better image quality and higher diagnostic accuracy compared to single-source transmit technology.

<sup>1</sup>Department of Internal Medicine/Cardiology, German Heart Institute Berlin, Berlin, Germany


Full list of author information is available at the end of the article

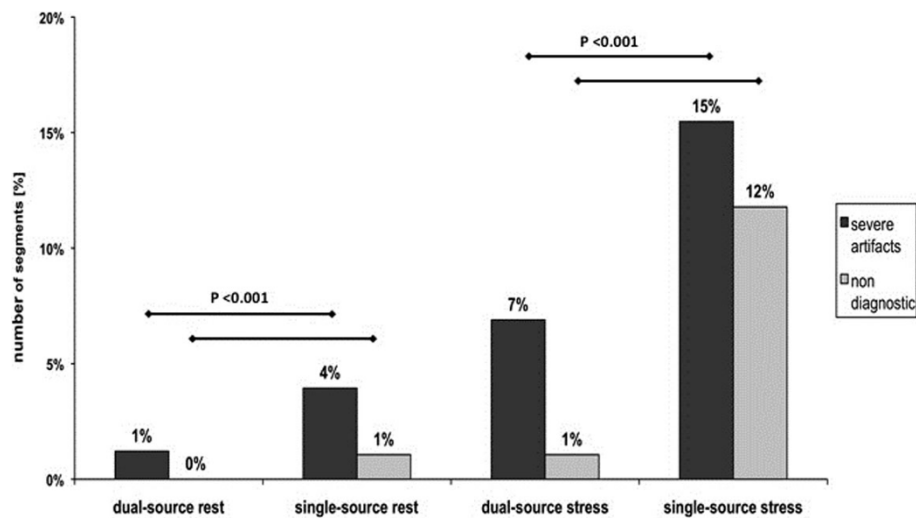

**Figure 1** Analysis of image quality of DSMR SSFP cine imaging at 3 Tesla. A significant difference existed between the number of segments with severe artifacts and no diagnostic segments comparing single-source and dual-source transmit technology both at rest and even more pronounced at maximum stress.

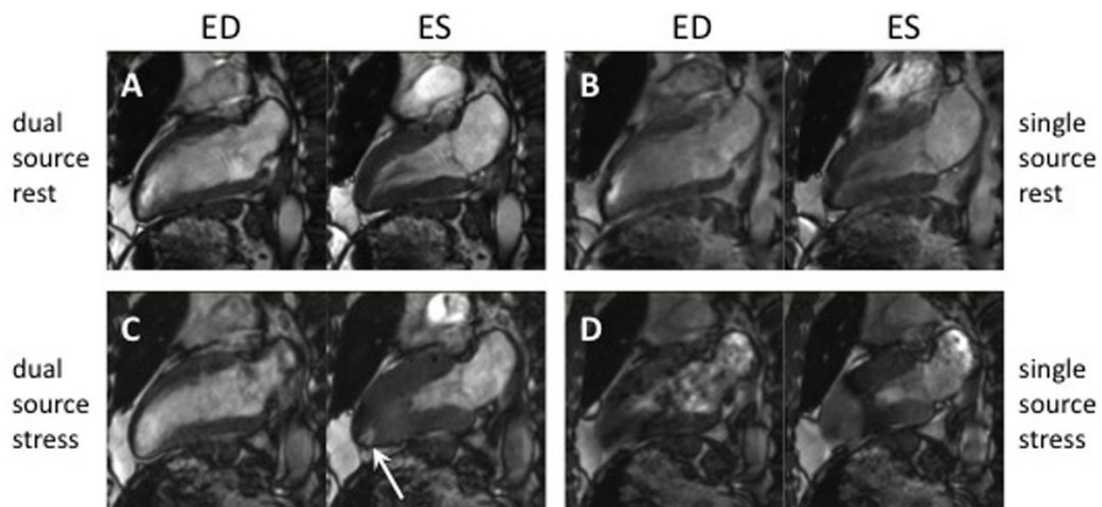

**Figure 2.** DSMR SSFP cine imaging at 3 Tesla using dual- vs. single source transmit technology. The single-source transmit technology is prone to banding artifacts especially at high heart rates leading to non diagnostic segments as seen on image D. A stress induced wall motion abnormality at the apex (white arrow) is visible during maximum stress using the dual source transmit technology (C). A high grade stenosis of the LAD (black arrow) is visualised by the corresponding patient's coronary angiogram (E).

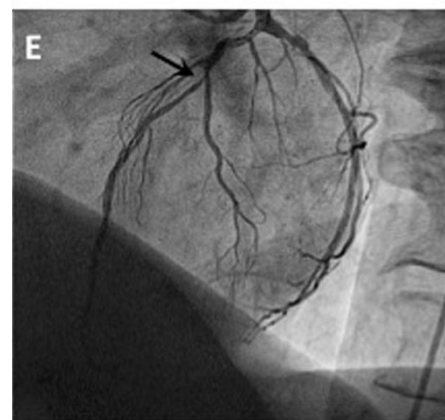

**Figure 2**

## Funding

None.

## Author details

<sup>1</sup>Department of Internal Medicine/Cardiology, German Heart Institute Berlin, Berlin, Germany. <sup>2</sup>Philips Healthcare, Hamburg, Germany. <sup>3</sup>Philips Healthcare, Best, Netherlands.

Published: 1 February 2012

doi:10.1186/1532-429X-14-S1-P252

**Cite this article as:** Berger *et al.*: High-dose dobutamine stress SSFP cine MRI at 3 Tesla with patient adaptive local RF shimming using dual-source RF transmission. *Journal of Cardiovascular Magnetic Resonance* 2012 **14**(Suppl 1):P252.

**Submit your next manuscript to BioMed Central  
and take full advantage of:**

- Convenient online submission
- Thorough peer review
- No space constraints or color figure charges
- Immediate publication on acceptance
- Inclusion in PubMed, CAS, Scopus and Google Scholar
- Research which is freely available for redistribution

Submit your manuscript at  
[www.biomedcentral.com/submit](http://www.biomedcentral.com/submit)

