

POSTER PRESENTATION

Open Access

Increased maximum gradient amplitude improves robustness of spin-echo cardiac diffusion-weighted MRI

Eric Aliotta^{1,2*}, Stanislas Rapacchi¹, Peng Hu^{1,2}, Daniel B Ennis^{1,2}

From 18th Annual SCMR Scientific Sessions
Nice, France. 4-7 February 2015

Background

Cardiac motion presents a major challenge in diffusion weighted MRI (DWI), often leading to large signal drop-outs that necessitate repeated measurements (Pai, V.M., *MRM* 2011). While cardiac DWI is generally ECG gated to apply diffusion weighting during peak-systole or end-diastole, these intervals can be short and difficult to pinpoint, resulting in poor sequence reproducibility.


Recent improvements in gradient hardware provide larger maximum gradients than current systems ($G_{\max}=80\text{mT/m}$), which can substantially reduce the temporal footprint of diffusion preparation and make cardiac DWI more robust to bulk motion.

Methods

A left ventricular (LV) motion model simulated motion of the healthy heart with 30-70ms quiescent intervals (t_Q). Monopolar encoded SE-DWI ($b=500\text{ s/mm}^2$, 3 directions) was simulated using: $G_{\max}=40$ and 80mT/m

with diffusion gradients centered at mid-quiescence and with a range temporal offsets ($\Delta T=\pm 20\text{ms}$). Complex Gaussian noise was added such that $\text{SNR}=50$ for $b=0$ images. Bulk motion induced error was measured by the bias in apparent diffusion coefficient (ADC) recovery from the programmed value ($\text{ADC}=1\times 10^{-3}\text{ mm}^2/\text{s}$). Sequences that recovered ADC with bias $<10\%$ for $\Delta T=\pm 10\text{ms}$ were deemed robust to motion.

Three healthy volunteers were scanned in a 3.0 T Siemens Prisma ($G_{\max}=80\text{mT/m}$) scanner using breath hold cardiac DWI (12 directions, monopolar encoding, single-shot SE EPI readout). Five repetitions of each sequence were acquired: 1) G40-b300: $G_{\max}=40\text{mT/m}$, $b=300\text{ mm}^2/\text{s}$, $\text{TE}=44\text{ms}$; 2) G40-b100: $G_{\max}=40\text{mT/m}$, $b=100\text{ mm}^2/\text{s}$, $\text{TE}=36\text{ms}$; and 3) G80-b300: $G_{\max}=80\text{mT/m}$, $b=300\text{ mm}^2/\text{s}$, $\text{TE}=36\text{ms}$. Imaging was timed to the diastolic quiescent interval, which was determined visually from CINE images.

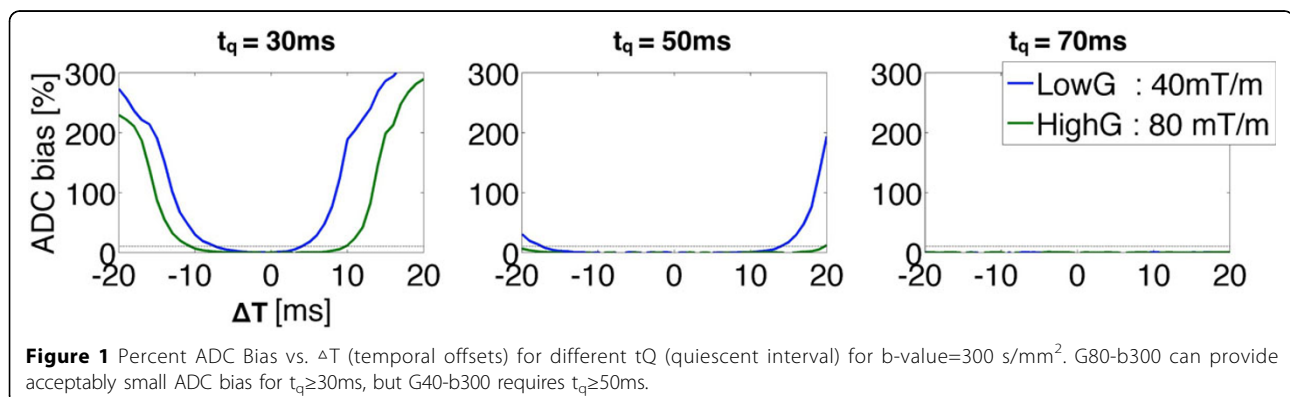

¹Radiology, UCLA, Los Angeles, CA, USA

Full list of author information is available at the end of the article

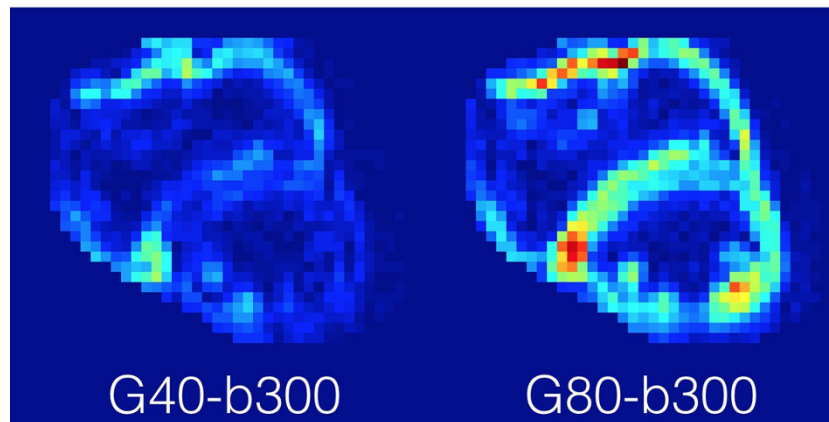


Figure 2 Typical DWI from G40-b300 (left) and G80-b300 (right). Image quality was generally better for G80-b300.

Two observers evaluated the quality of all images as: “acceptable”-no significant signal dropouts in myocardium or “unacceptable”-significant signal dropouts, and directly compared G40-b300 to G80-b300 (fixed b-value).

Results

The simulated ADC bias (Fig. 1) shows that G80-b300 can provide acceptably small ADC bias for $t_Q \geq 30$ ms, but G40-b300 requires $t_Q \geq 50$ ms.

Image quality was better in G80-b300 than G40-b300 in 86% of images (example pair shown in Figure 2). 55% of G80-b300 images were acceptable, whereas 30% of G40-b300 and 70% of G40-b100 were.

Conclusions

Simulations show that G80 recovered ADC more accurately than G40 for all t_Q and ΔT and was robust to motion for $t_Q \geq 30$ ms. This is likely due to the shorter diffusion preparation (G40 $t_{prep}=39$ ms, G80 $t_{prep}=28$ ms) and indicates that G80 will perform more consistently for short t_Q (fast heart rates, systolic imaging) or changes in heart rhythm.

With fixed b-value= $300\text{mm}^2/\text{s}$ in vivo, G80 had consistently better image quality than G40. In agreement with simulation, this indicates that G80 improves the robustness of cardiac DWI for the same b-value. With fixed TE=36ms, G40-b100 was acceptable more frequently than G80-b300, but with insufficient diffusion weighting. Increased G_{max} can thus improve diffusion sensitivity with less loss of robustness.

Funding

This research was supported by Siemens Medical Solutions and the Department of Radiological Sciences at UCLA.

Authors' details

¹Radiology, UCLA, Los Angeles, CA, USA. ²Biomedical Physics IDP, UCLA, Los Angeles, CA, USA.

Published: 3 February 2015

doi:10.1186/1532-429X-17-S1-P388

Cite this article as: Aliotta et al.: Increased maximum gradient amplitude improves robustness of spin-echo cardiac diffusion-weighted MRI. *Journal of Cardiovascular Magnetic Resonance* 2015 17(Suppl 1):P388.

Submit your next manuscript to BioMed Central and take full advantage of:

- Convenient online submission
- Thorough peer review
- No space constraints or color figure charges
- Immediate publication on acceptance
- Inclusion in PubMed, CAS, Scopus and Google Scholar
- Research which is freely available for redistribution

Submit your manuscript at
www.biomedcentral.com/submit

